




**Ohaus Corporation**  
29 Hanover Road  
Florham Park, NJ  
07932-0900

# Operating instructions

*Voyager balances*

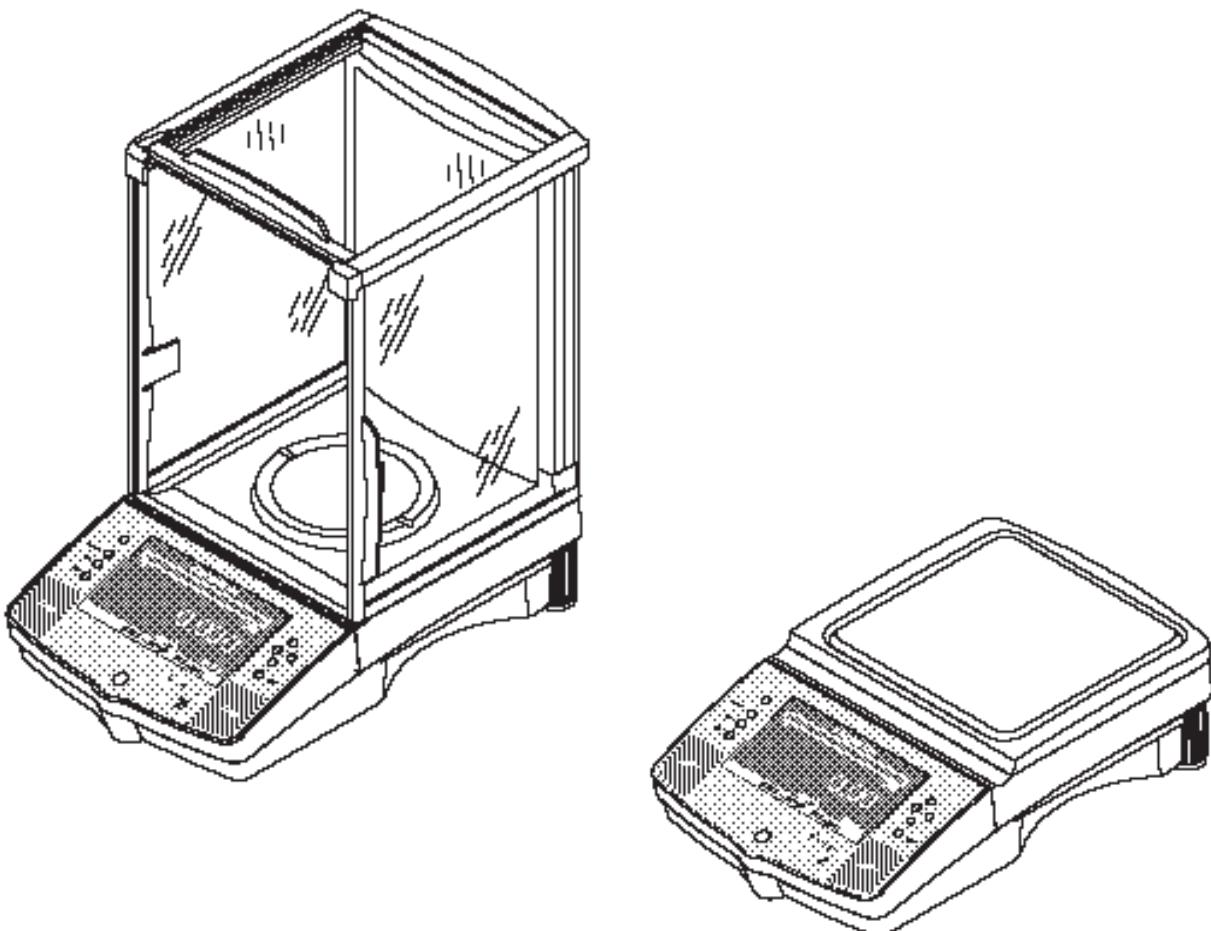

# Contents

OVERVIEW OF CONTROLS .....	8
<b>1. GETTING TO KNOW YOUR VOYAGER BALANCE .....</b>	<b>9</b>
1.1 Introduction .....	9
1.2 Overview of the Voyager balance .....	9
1.3 What you should know about these instructions .....	10
1.4 Safety is first .....	10
<b>2. INSTALLATION .....</b>	<b>11</b>
2.1 Unpacking and checking the standard equipment .....	11
2.2 Selecting the location .....	12
2.3 Leveling the balance .....	12
2.4 Installing cover plate and pan .....	12
2.5 Installing wind shield .....	13
2.6 Power supply .....	13
2.7 Switching the balance on or off .....	14
2.8 Weigh below preparation .....	14
<b>3. THE MENU .....</b>	<b>15</b>
3.1 What is the menu? .....	15
3.2 Menu operation .....	16
3.3 Library .....	17
<b>4. CALIBRATION .....</b>	<b>18</b>
4.1 Span calibration .....	20
4.2 Linearity calibration .....	21
4.3 User calibration .....	22
4.4 Calibration test .....	23
4.5 Auto calibration .....	24
4.6 AutoCal™ delta correction .....	25

<b>5. WEIGHING MADE SIMPLE .....</b>	<b>26</b>
5.1 Selecting a weighing unit .....	26
5.2 Taring the balance .....	27
5.3 Performing a simple weighing .....	27
5.4 Custom unit .....	28
<b>6. BALANCE MODES .....</b>	<b>31</b>
6.1 Parts counting .....	31
6.1.1 Easy count .....	31
6.1.2 Advanced counting .....	32
6.2 Filling .....	33
6.3 Animal weighing .....	34
6.4 Check weighing .....	35
6.5 Differential weighing .....	36
6.6 Formulation .....	41
6.7 Quick check weighing .....	43
6.8 Statistics/function link .....	44
6.9 Density .....	45
6.9.1 Balance preparation with density kit .....	45
6.9.2 Solid density determination for items more dense than water .....	46
6.9.3 Solid density determination for items less dense than water .....	48
6.9.4 Improving the accuracy of the result of solid density .....	49
6.9.5 Liquid density determination .....	50
6.10 Statistical quality control (SQC) .....	51
6.10.1 Resuming a particular SQC setup .....	54
6.10.2 Specifying a new SQC setup .....	55
6.10.3 Redoing or correcting a batch .....	56
6.11 Pipette calibration .....	57
<b>7. BALANCE SETTINGS .....</b>	<b>62</b>
7.1 Reset to factory settings .....	62
7.2 Setting contrast and brightness of the display .....	62
7.3 Setting the readout .....	63
7.4 Setting the interface .....	64
7.5 Setting print option .....	65

7.6	Setting GLP print options .....	66
7.7	Setting time and date .....	67
7.8	Setting auto calibration .....	68
7.9	Print current settings .....	68
7.10	Lock out .....	
69		
7.11	Software version .....	70
7.12	Setting custom menu .....	70
7.13	Legal for trade .....	71
7.14	Menu lock-out protection .....	72
<b>8.</b>	<b>RS232 INTERFACE/PRINTING DATA .....</b>	<b>73</b>
8.1	RS232 interface .....	73
8.2	Printing data .....	76
<b>9.</b>	<b>CARE AND MAINTENANCE .....</b>	<b>79</b>
9.1	Troubleshooting .....	79
9.2	Error codes list .....	80
9.3	Information messages .....	81
9.4	Service information .....	81
9.5	Replacement parts .....	81
9.6	Accessories .....	81
9.7	Specifications .....	82
<b>A</b>	<b>APPENDIX SPECIAL APPLICATIONS .....</b>	<b>83</b>
A-1	Sieve analysis .....	83
A-2	Porous material density determinations .....	86

This is a “Table of Contents preview” for quality assurance

The full manual can be purchased from our store:

[https://the-checkout-tech.com/manuals/ohaus/Voyager user manual.html](https://the-checkout-tech.com/manuals/ohaus/Voyager%20user%20manual.html)

And our free Online Keysheet maker:

<https://the-checkout-tech.com/Cash-Register-Keysheet-Creator/>

[HTTPS://THE-CHECKOUT-TECH.COM](https://THE-CHECKOUT-TECH.COM)